


AG2.5 Refractometer Calibration Fluid Refractive Index Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	1.33739	1.33739	1.33738	1.33737	1.33737	1.33736	1.33735	1.33735	1.33734	1.33733
11	1.33732	1.33732	1.33731	1.33730	1.33730	1.33729	1.33728	1.33728	1.33727	1.33726
12	1.33725	1.33725	1.33724	1.33723	1.33722	1.33722	1.33721	1.33720	1.33720	1.33719
13	1.33718	1.33717	1.33717	1.33716	1.33715	1.33714	1.33714	1.33713	1.33712	1.33711
14	1.33710	1.33710	1.33709	1.33708	1.33707	1.33707	1.33706	1.33705	1.33704	1.33703
15	1.33703	1.33702	1.33701	1.33700	1.33699	1.33699	1.33698	1.33697	1.33696	1.33695
16	1.33694	1.33694	1.33693	1.33692	1.33691	1.33690	1.33689	1.33689	1.33688	1.33687
17	1.33686	1.33685	1.33684	1.33683	1.33683	1.33682	1.33681	1.33680	1.33679	1.33678
18	1.33677	1.33676	1.33676	1.33675	1.33674	1.33673	1.33672	1.33671	1.33670	1.33669
19	1.33668	1.33667	1.33667	1.33666	1.33665	1.33664	1.33663	1.33662	1.33661	1.33660
20	1.33659	1.33658	1.33657	1.33656	1.33655	1.33654	1.33653	1.33652	1.33651	1.33651
21	1.33650	1.33649	1.33648	1.33647	1.33646	1.33645	1.33644	1.33643	1.33642	1.33641
22	1.33640	1.33639	1.33638	1.33637	1.33636	1.33635	1.33634	1.33633	1.33632	1.33631
23	1.33630	1.33628	1.33627	1.33626	1.33625	1.33624	1.33623	1.33622	1.33621	1.33620
24	1.33619	1.33618	1.33617	1.33616	1.33615	1.33614	1.33613	1.33612	1.33610	1.33609
25	1.33608	1.33607	1.33606	1.33605	1.33604	1.33603	1.33602	1.33601	1.33599	1.33598
26	1.33597	1.33596	1.33595	1.33594	1.33593	1.33592	1.33590	1.33589	1.33588	1.33587
27	1.33586	1.33585	1.33583	1.33582	1.33581	1.33580	1.33579	1.33578	1.33576	1.33575
28	1.33574	1.33573	1.33572	1.33570	1.33569	1.33568	1.33567	1.33566	1.33564	1.33563
29	1.33562	1.33561	1.33559	1.33558	1.33557	1.33556	1.33555	1.33553	1.33552	1.33551
30	1.33550	1.33548	1.33547	1.33546	1.33544	1.33543	1.33542	1.33541	1.33539	1.33538
31	1.33537	1.33535	1.33534	1.33533	1.33532	1.33530	1.33529	1.33528	1.33526	1.33525
32	1.33524	1.33522	1.33521	1.33520	1.33518	1.33517	1.33516	1.33514	1.33513	1.33512
33	1.33510	1.33509	1.33508	1.33506	1.33505	1.33503	1.33502	1.33501	1.33499	1.33498
34	1.33496	1.33495	1.33494	1.33492	1.33491	1.33489	1.33488	1.33487	1.33485	1.33484
35	1.33482	1.33481	1.33479	1.33478	1.33477	1.33475	1.33474	1.33472	1.33471	1.33469
36	1.33468	1.33466	1.33465	1.33463	1.33462	1.33460	1.33459	1.33457	1.33456	1.33454
37	1.33453	1.33451	1.33450	1.33448	1.33447	1.33445	1.33444	1.33442	1.33441	1.33439
38	1.33438	1.33436	1.33435	1.33433	1.33431	1.33430	1.33428	1.33427	1.33425	1.33424
39	1.33422	1.33420	1.33419	1.33417	1.33416	1.33414	1.33413	1.33411	1.33409	1.33408
40	1.33406									

AG2.5 Refractometer Calibration Fluid - R.I. Temperature Relationship

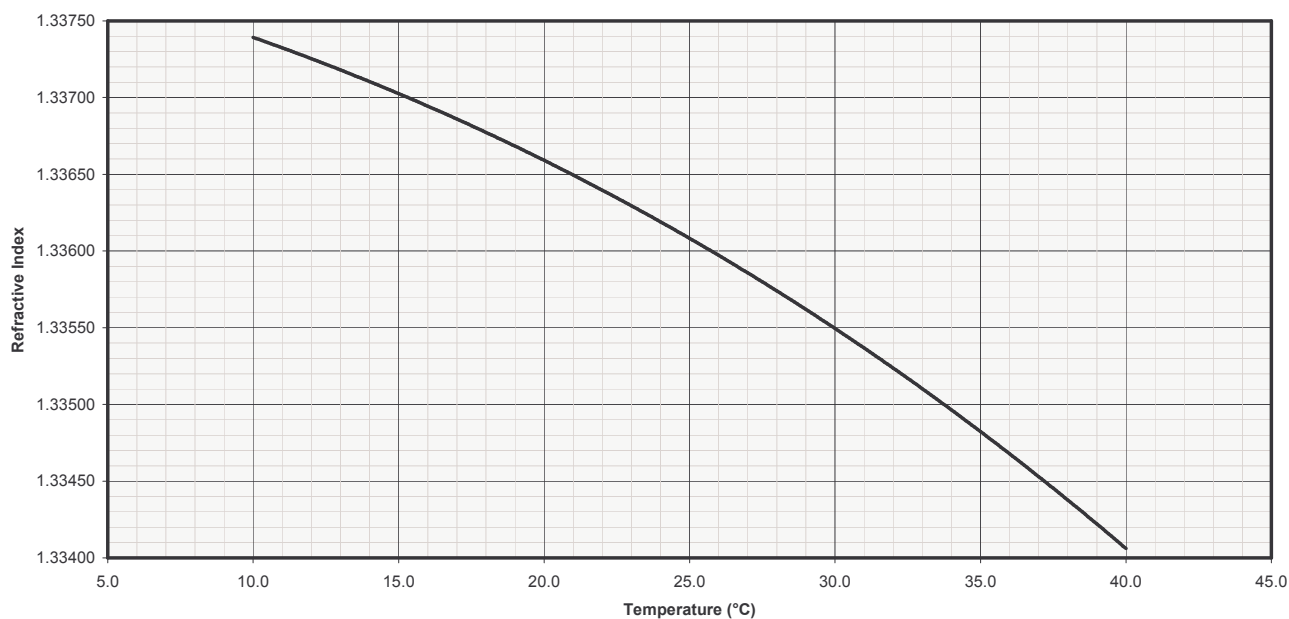

Code: 90-303 Issue: 1



Bellingham + Stanley Ltd.

Longfield Road, Tunbridge Wells
 KENT. TN2 3EY
 UK
 Telephone: +44 (0) 1892 500400
 Fax: +44 (0) 1892 543115


Bellingham + Stanley Inc.

1000 Hurricane Shoals Road
 Bldg D, Suite 300
 LAWRENCEVILLE, USA, GA 30043
 Telephone: 770 822 6898
 Fax: 770 822 9165

AG2.5 Refractometer Calibration Fluid °Brix Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	3.05	3.05	3.04	3.04	3.03	3.03	3.02	3.02	3.01	3.01
11	3.00	3.00	2.99	2.99	2.98	2.98	2.97	2.97	2.96	2.96
12	2.95	2.95	2.94	2.94	2.93	2.93	2.92	2.92	2.91	2.91
13	2.90	2.90	2.89	2.89	2.88	2.88	2.87	2.87	2.86	2.86
14	2.85	2.85	2.84	2.84	2.83	2.83	2.82	2.82	2.81	2.80
15	2.80	2.79	2.79	2.78	2.78	2.77	2.77	2.76	2.75	2.75
16	2.74	2.74	2.73	2.73	2.72	2.71	2.71	2.70	2.70	2.69
17	2.69	2.68	2.67	2.67	2.66	2.66	2.65	2.64	2.64	2.63
18	2.63	2.62	2.61	2.61	2.60	2.60	2.59	2.58	2.58	2.57
19	2.56	2.56	2.55	2.55	2.54	2.53	2.53	2.52	2.51	2.51
20	2.50	2.49	2.49	2.48	2.47	2.47	2.46	2.46	2.45	2.44
21	2.44	2.43	2.42	2.42	2.41	2.40	2.39	2.39	2.38	2.37
22	2.37	2.36	2.35	2.35	2.34	2.33	2.33	2.32	2.31	2.30
23	2.30	2.29	2.28	2.28	2.27	2.26	2.25	2.25	2.24	2.23
24	2.23	2.22	2.21	2.20	2.20	2.19	2.18	2.17	2.17	2.16
25	2.15	2.14	2.14	2.13	2.12	2.11	2.11	2.10	2.09	2.08
26	2.08	2.07	2.06	2.05	2.04	2.04	2.03	2.02	2.01	2.00
27	2.00	1.99	1.98	1.97	1.96	1.96	1.95	1.94	1.93	1.92
28	1.92	1.91	1.90	1.89	1.88	1.87	1.87	1.86	1.85	1.84
29	1.83	1.82	1.82	1.81	1.80	1.79	1.78	1.77	1.76	1.76
30	1.75	1.74	1.73	1.72	1.71	1.70	1.69	1.69	1.68	1.67
31	1.66	1.65	1.64	1.63	1.62	1.61	1.60	1.60	1.59	1.58
32	1.57	1.56	1.55	1.54	1.53	1.52	1.51	1.50	1.49	1.48
33	1.48	1.47	1.46	1.45	1.44	1.43	1.42	1.41	1.40	1.39
34	1.38	1.37	1.36	1.35	1.34	1.33	1.32	1.31	1.30	1.29
35	1.28	1.27	1.26	1.25	1.24	1.23	1.22	1.21	1.20	1.19
36	1.18	1.17	1.16	1.15	1.14	1.13	1.12	1.11	1.10	1.09
37	1.08	1.07	1.06	1.05	1.04	1.03	1.02	1.00	0.99	0.98
38	0.97	0.96	0.95	0.94	0.93	0.92	0.91	0.90	0.89	0.88
39	0.86	0.85	0.84	0.83	0.82	0.81	0.80	0.79	0.78	0.76
40	0.75									

AG2.5 Refractometer Calibration Fluid - °Brix Temperature Relationship

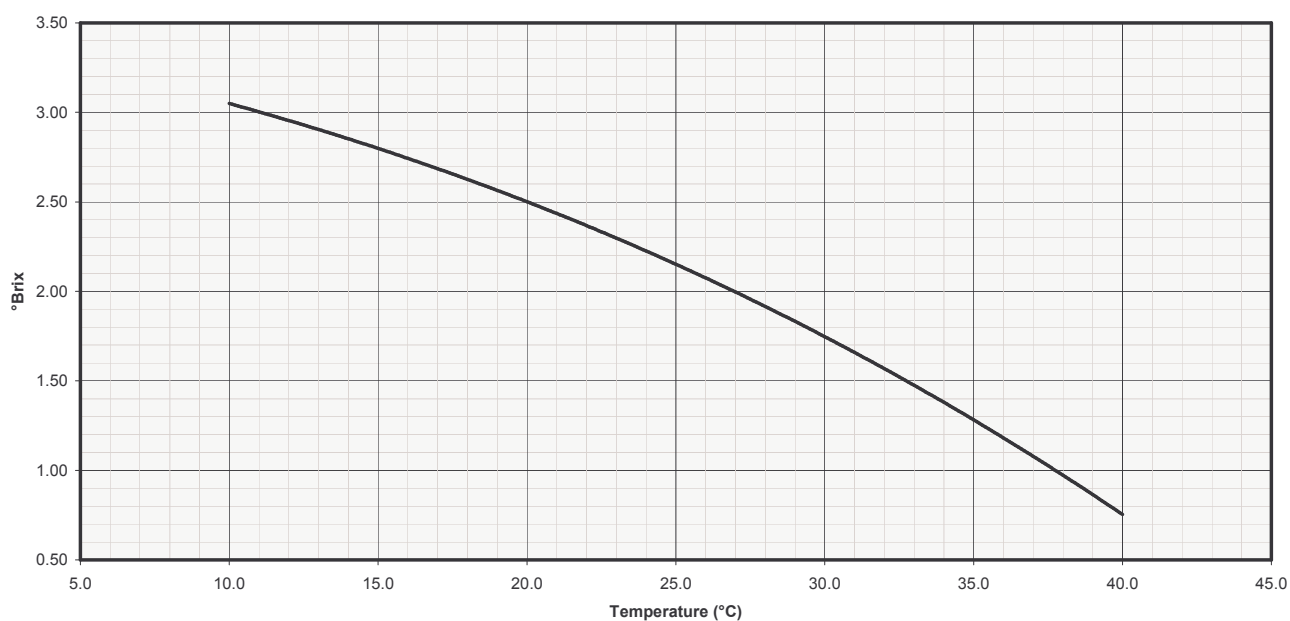

Code: 90-303 Issue: 1



Bellingham + Stanley Ltd.

Longfield Road, Tunbridge Wells
 KENT. TN2 3EY
 UK
 Telephone: +44 (0) 1892 500400
 Fax: +44 (0) 1892 543115

Bellingham + Stanley Inc.

1000 Hurricane Shoals Road
 Bldg D, Suite 300
 LAWRENCEVILLE, USA, GA 30043
 Telephone: 770 822 6898
 Fax: 770 822 9165