


AG7.5 Refractometer Calibration Fluid Refractive Index Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	1.34496	1.34495	1.34494	1.34493	1.34492	1.34492	1.34491	1.34490	1.34489	1.34488
11	1.34487	1.34487	1.34486	1.34485	1.34484	1.34483	1.34482	1.34481	1.34481	1.34480
12	1.34479	1.34478	1.34477	1.34476	1.34475	1.34474	1.34474	1.34473	1.34472	1.34471
13	1.34470	1.34469	1.34468	1.34467	1.34466	1.34465	1.34465	1.34464	1.34463	1.34462
14	1.34461	1.34460	1.34459	1.34458	1.34457	1.34456	1.34455	1.34454	1.34453	1.34452
15	1.34451	1.34451	1.34450	1.34449	1.34448	1.34447	1.34446	1.34445	1.34444	1.34443
16	1.34442	1.34441	1.34440	1.34439	1.34438	1.34437	1.34436	1.34435	1.34434	1.34433
17	1.34432	1.34431	1.34430	1.34429	1.34428	1.34427	1.34426	1.34425	1.34424	1.34423
18	1.34422	1.34421	1.34420	1.34419	1.34418	1.34417	1.34416	1.34415	1.34414	1.34413
19	1.34412	1.34410	1.34409	1.34408	1.34407	1.34406	1.34405	1.34404	1.34403	1.34402
20	1.34401	1.34400	1.34399	1.34398	1.34397	1.34395	1.34394	1.34393	1.34392	1.34391
21	1.34390	1.34389	1.34388	1.34387	1.34385	1.34384	1.34383	1.34382	1.34381	1.34380
22	1.34379	1.34378	1.34376	1.34375	1.34374	1.34373	1.34372	1.34371	1.34369	1.34368
23	1.34367	1.34366	1.34365	1.34364	1.34362	1.34361	1.34360	1.34359	1.34358	1.34357
24	1.34355	1.34354	1.34353	1.34352	1.34351	1.34349	1.34348	1.34347	1.34346	1.34344
25	1.34343	1.34342	1.34341	1.34340	1.34338	1.34337	1.34336	1.34335	1.34333	1.34332
26	1.34331	1.34330	1.34328	1.34327	1.34326	1.34325	1.34323	1.34322	1.34321	1.34319
27	1.34318	1.34317	1.34316	1.34314	1.34313	1.34312	1.34310	1.34309	1.34308	1.34306
28	1.34305	1.34304	1.34303	1.34301	1.34300	1.34299	1.34297	1.34296	1.34295	1.34293
29	1.34292	1.34290	1.34289	1.34288	1.34286	1.34285	1.34284	1.34282	1.34281	1.34280
30	1.34278	1.34277	1.34275	1.34274	1.34273	1.34271	1.34270	1.34268	1.34267	1.34266
31	1.34264	1.34263	1.34261	1.34260	1.34259	1.34257	1.34256	1.34254	1.34253	1.34251
32	1.34250	1.34248	1.34247	1.34246	1.34244	1.34243	1.34241	1.34240	1.34238	1.34237
33	1.34235	1.34234	1.34232	1.34231	1.34229	1.34228	1.34226	1.34225	1.34223	1.34222
34	1.34220	1.34219	1.34217	1.34216	1.34214	1.34213	1.34211	1.34210	1.34208	1.34207
35	1.34205	1.34204	1.34202	1.34200	1.34199	1.34197	1.34196	1.34194	1.34193	1.34191
36	1.34189	1.34188	1.34186	1.34185	1.34183	1.34181	1.34180	1.34178	1.34177	1.34175
37	1.34173	1.34172	1.34170	1.34169	1.34167	1.34165	1.34164	1.34162	1.34160	1.34159
38	1.34157	1.34155	1.34154	1.34152	1.34150	1.34149	1.34147	1.34145	1.34144	1.34142
39	1.34140	1.34139	1.34137	1.34135	1.34134	1.34132	1.34130	1.34128	1.34127	1.34125
40	1.34123									

AG7.5 Refractometer Calibration Fluid - R.I. Temperature Relationship

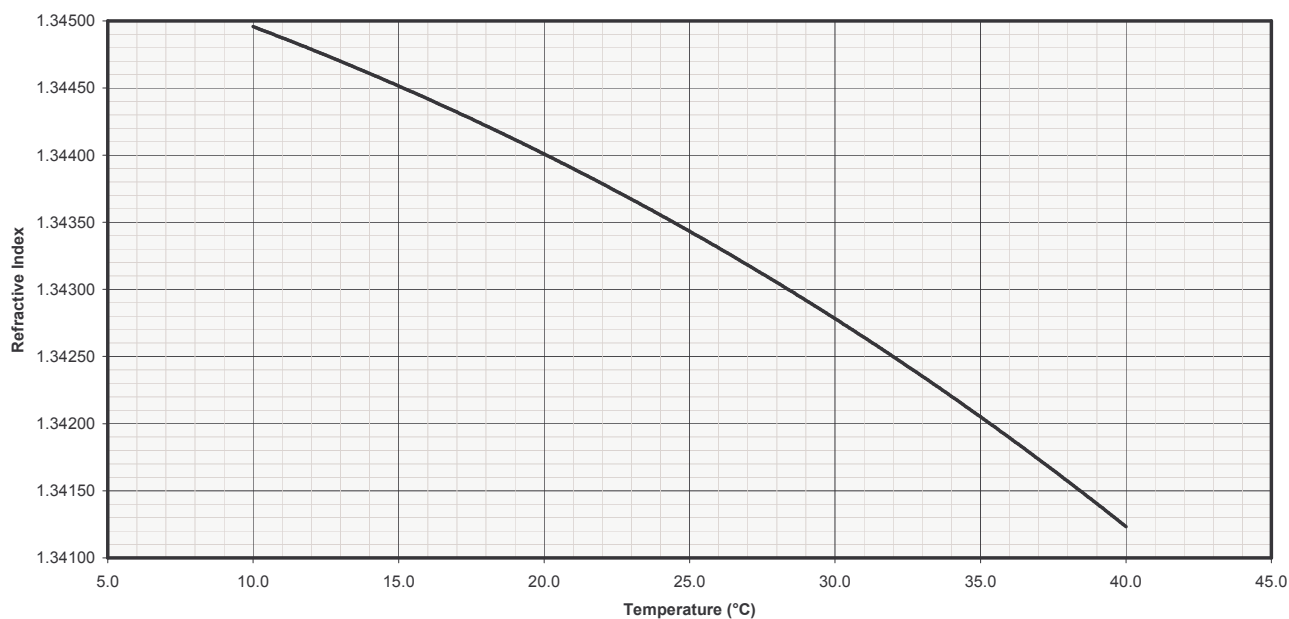

Code: 90-305 Issue: 1



Bellingham + Stanley Ltd.

Longfield Road, Tunbridge Wells

KENT. TN2 3EY

UK

Telephone: +44 (0) 1892 500400

Fax: +44 (0) 1892 543115

Bellingham + Stanley Inc.

1000 Hurricane Shoals Road

Bldg D, Suite 300

LAWRENCEVILLE, USA, GA 30043


Telephone: 770 822 6898

Fax: 770 822 9165

AG7.5 Refractometer Calibration Fluid °Brix Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	8.12	8.12	8.11	8.11	8.10	8.10	8.09	8.08	8.08	8.07
11	8.07	8.06	8.06	8.05	8.05	8.04	8.03	8.03	8.02	8.02
12	8.01	8.01	8.00	7.99	7.99	7.98	7.98	7.97	7.96	7.96
13	7.95	7.95	7.94	7.94	7.93	7.92	7.92	7.91	7.91	7.90
14	7.89	7.89	7.88	7.87	7.87	7.86	7.86	7.85	7.84	7.84
15	7.83	7.83	7.82	7.81	7.81	7.80	7.79	7.79	7.78	7.77
16	7.77	7.76	7.76	7.75	7.74	7.74	7.73	7.72	7.72	7.71
17	7.70	7.70	7.69	7.68	7.68	7.67	7.66	7.66	7.65	7.64
18	7.64	7.63	7.62	7.62	7.61	7.60	7.60	7.59	7.58	7.57
19	7.57	7.56	7.55	7.55	7.54	7.53	7.53	7.52	7.51	7.50
20	7.50	7.49	7.48	7.48	7.47	7.46	7.45	7.45	7.44	7.43
21	7.42	7.42	7.41	7.40	7.40	7.39	7.38	7.37	7.37	7.36
22	7.35	7.34	7.34	7.33	7.32	7.31	7.30	7.30	7.29	7.28
23	7.27	7.27	7.26	7.25	7.24	7.24	7.23	7.22	7.21	7.20
24	7.20	7.19	7.18	7.17	7.16	7.16	7.15	7.14	7.13	7.12
25	7.12	7.11	7.10	7.09	7.08	7.07	7.07	7.06	7.05	7.04
26	7.03	7.03	7.02	7.01	7.00	6.99	6.98	6.97	6.97	6.96
27	6.95	6.94	6.93	6.92	6.91	6.91	6.90	6.89	6.88	6.87
28	6.86	6.85	6.85	6.84	6.83	6.82	6.81	6.80	6.79	6.78
29	6.77	6.77	6.76	6.75	6.74	6.73	6.72	6.71	6.70	6.69
30	6.68	6.67	6.67	6.66	6.65	6.64	6.63	6.62	6.61	6.60
31	6.59	6.58	6.57	6.56	6.55	6.54	6.53	6.52	6.51	6.50
32	6.50	6.49	6.48	6.47	6.46	6.45	6.44	6.43	6.42	6.41
33	6.40	6.39	6.38	6.37	6.36	6.35	6.34	6.33	6.32	6.31
34	6.30	6.29	6.28	6.27	6.26	6.25	6.24	6.23	6.22	6.21
35	6.20	6.19	6.18	6.16	6.15	6.14	6.13	6.12	6.11	6.10
36	6.09	6.08	6.07	6.06	6.05	6.04	6.03	6.02	6.01	6.00
37	5.98	5.97	5.96	5.95	5.94	5.93	5.92	5.91	5.90	5.89
38	5.88	5.86	5.85	5.84	5.83	5.82	5.81	5.80	5.79	5.77
39	5.76	5.75	5.74	5.73	5.72	5.71	5.70	5.68	5.67	5.66
40	5.65									

AG7.5 Refractometer Calibration Fluid - °Brix Temperature Relationship

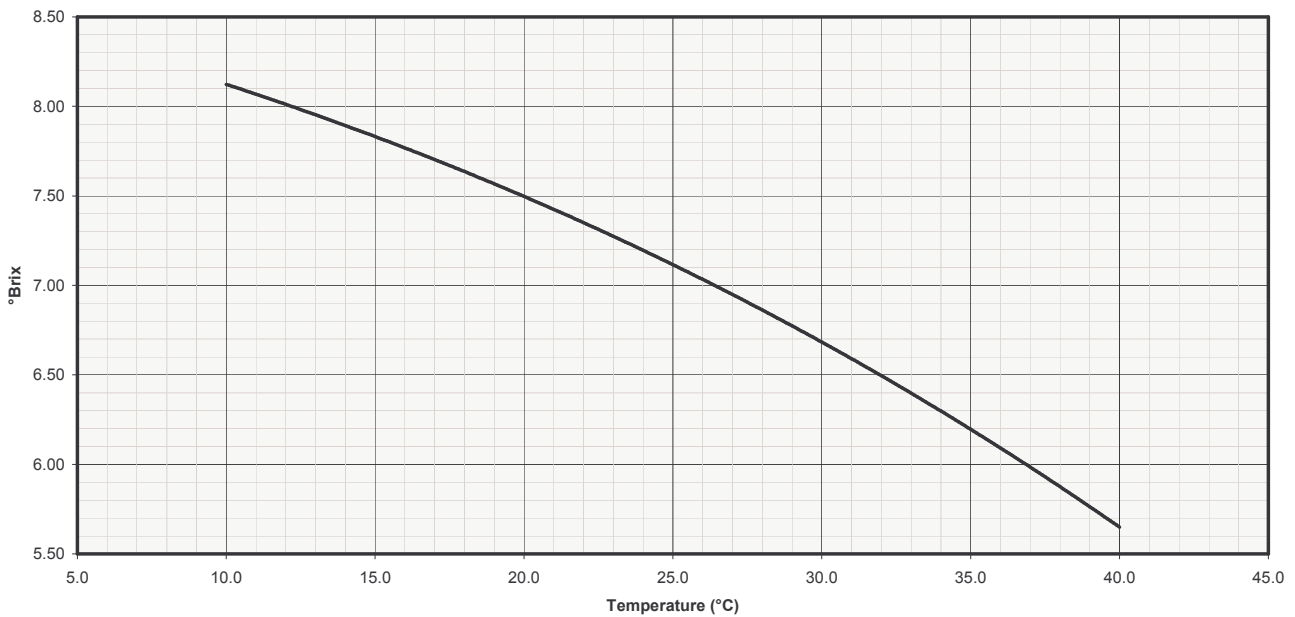

Code: 90-305 Issue: 1



Bellingham + Stanley Ltd.

Longfield Road, Tunbridge Wells
 KENT. TN2 3EY
 UK
 Telephone: +44 (0) 1892 500400
 Fax: +44 (0) 1892 543115

Bellingham + Stanley Inc.

1000 Hurricane Shoals Road
 Bldg D, Suite 300
 LAWRENCEVILLE, USA, GA 30043
 Telephone: 770 822 6898
 Fax: 770 822 9165