


## AG2.5 Refractometer Calibration Fluid Refractive Index Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	1.33739	1.33739	1.33738	1.33737	1.33737	1.33736	1.33735	1.33735	1.33734	1.33733
11	1.33732	1.33732	1.33731	1.33730	1.33730	1.33729	1.33728	1.33728	1.33727	1.33726
12	1.33725	1.33725	1.33724	1.33723	1.33722	1.33722	1.33721	1.33720	1.33720	1.33719
13	1.33718	1.33717	1.33717	1.33716	1.33715	1.33714	1.33714	1.33713	1.33712	1.33711
14	1.33710	1.33710	1.33709	1.33708	1.33707	1.33707	1.33706	1.33705	1.33704	1.33703
15	1.33703	1.33702	1.33701	1.33700	1.33699	1.33699	1.33698	1.33697	1.33696	1.33695
16	1.33694	1.33694	1.33693	1.33692	1.33691	1.33690	1.33689	1.33689	1.33688	1.33687
17	1.33686	1.33685	1.33684	1.33683	1.33683	1.33682	1.33681	1.33680	1.33679	1.33678
18	1.33677	1.33676	1.33676	1.33675	1.33674	1.33673	1.33672	1.33671	1.33670	1.33669
19	1.33668	1.33667	1.33667	1.33666	1.33665	1.33664	1.33663	1.33662	1.33661	1.33660
20	1.33659	1.33658	1.33657	1.33656	1.33655	1.33654	1.33653	1.33652	1.33651	1.33651
21	1.33650	1.33649	1.33648	1.33647	1.33646	1.33645	1.33644	1.33643	1.33642	1.33641
22	1.33640	1.33639	1.33638	1.33637	1.33636	1.33635	1.33634	1.33633	1.33632	1.33631
23	1.33630	1.33628	1.33627	1.33626	1.33625	1.33624	1.33623	1.33622	1.33621	1.33620
24	1.33619	1.33618	1.33617	1.33616	1.33615	1.33614	1.33613	1.33612	1.33610	1.33609
25	1.33608	1.33607	1.33606	1.33605	1.33604	1.33603	1.33602	1.33601	1.33599	1.33598
26	1.33597	1.33596	1.33595	1.33594	1.33593	1.33592	1.33590	1.33589	1.33588	1.33587
27	1.33586	1.33585	1.33583	1.33582	1.33581	1.33580	1.33579	1.33578	1.33576	1.33575
28	1.33574	1.33573	1.33572	1.33570	1.33569	1.33568	1.33567	1.33566	1.33564	1.33563
29	1.33562	1.33561	1.33559	1.33558	1.33557	1.33556	1.33555	1.33553	1.33552	1.33551
30	1.33550	1.33548	1.33547	1.33546	1.33544	1.33543	1.33542	1.33541	1.33539	1.33538
31	1.33537	1.33535	1.33534	1.33533	1.33532	1.33530	1.33529	1.33528	1.33526	1.33525
32	1.33524	1.33522	1.33521	1.33520	1.33518	1.33517	1.33516	1.33514	1.33513	1.33512
33	1.33510	1.33509	1.33508	1.33506	1.33505	1.33503	1.33502	1.33501	1.33499	1.33498
34	1.33496	1.33495	1.33494	1.33492	1.33491	1.33489	1.33488	1.33487	1.33485	1.33484
35	1.33482	1.33481	1.33479	1.33478	1.33477	1.33475	1.33474	1.33472	1.33471	1.33469
36	1.33468	1.33466	1.33465	1.33463	1.33462	1.33460	1.33459	1.33457	1.33456	1.33454
37	1.33453	1.33451	1.33450	1.33448	1.33447	1.33445	1.33444	1.33442	1.33441	1.33439
38	1.33438	1.33436	1.33435	1.33433	1.33431	1.33430	1.33428	1.33427	1.33425	1.33424
39	1.33422	1.33420	1.33419	1.33417	1.33416	1.33414	1.33413	1.33411	1.33409	1.33408
40	1.33406									

**AG2.5 Refractometer Calibration Fluid - R.I. Temperature Relationship**

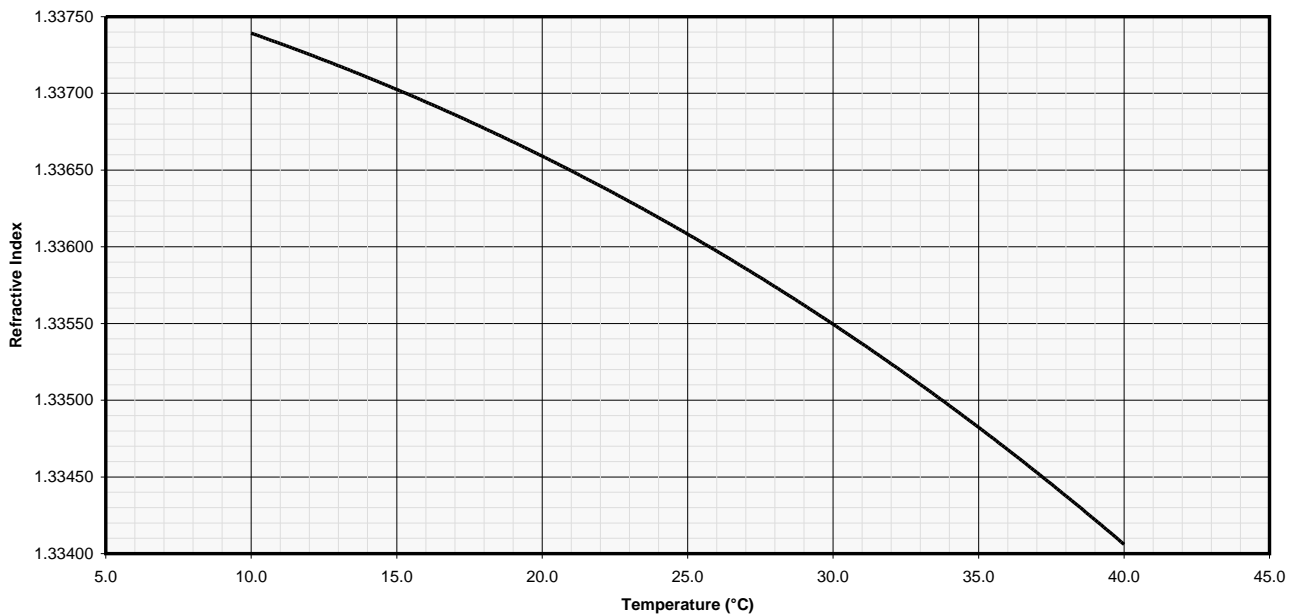

Code: 90-303 Issue: 02 Revision: A



**Bellingham + Stanley Ltd.**

Longfield Road  
Tunbridge Wells  
Kent, TN2 3EY, UK  
Telephone: +44 (0) 1892 500400  
Fax: +44 (0) 1892 543115


**Bellingham + Stanley Inc.**

90 Horizon Drive  
Suwanee  
GA 30024, USA  
Telephone: 678 804 5730  
Fax: 678 804 5729

## AG2.5 Refractometer Calibration Fluid °Brix Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	3.05	3.05	3.04	3.04	3.03	3.03	3.02	3.02	3.01	3.01
11	3.00	3.00	2.99	2.99	2.98	2.98	2.97	2.97	2.96	2.96
12	2.95	2.95	2.94	2.94	2.93	2.93	2.92	2.92	2.91	2.91
13	2.90	2.90	2.89	2.89	2.88	2.88	2.87	2.87	2.86	2.86
14	2.85	2.85	2.84	2.84	2.83	2.83	2.82	2.82	2.81	2.80
15	2.80	2.79	2.79	2.78	2.78	2.77	2.77	2.76	2.75	2.75
16	2.74	2.74	2.73	2.73	2.72	2.71	2.71	2.70	2.70	2.69
17	2.69	2.68	2.67	2.67	2.66	2.66	2.65	2.64	2.64	2.63
18	2.63	2.62	2.61	2.61	2.60	2.60	2.59	2.58	2.58	2.57
19	2.56	2.56	2.55	2.55	2.54	2.53	2.53	2.52	2.51	2.51
20	2.50	2.49	2.49	2.48	2.47	2.47	2.46	2.46	2.45	2.44
21	2.44	2.43	2.42	2.42	2.41	2.40	2.39	2.39	2.38	2.37
22	2.37	2.36	2.35	2.35	2.34	2.33	2.33	2.32	2.31	2.30
23	2.30	2.29	2.28	2.28	2.27	2.26	2.25	2.25	2.24	2.23
24	2.23	2.22	2.21	2.20	2.20	2.19	2.18	2.17	2.17	2.16
25	2.15	2.14	2.14	2.13	2.12	2.11	2.11	2.10	2.09	2.08
26	2.08	2.07	2.06	2.05	2.04	2.04	2.03	2.02	2.01	2.00
27	2.00	1.99	1.98	1.97	1.96	1.96	1.95	1.94	1.93	1.92
28	1.92	1.91	1.90	1.89	1.88	1.87	1.87	1.86	1.85	1.84
29	1.83	1.82	1.82	1.81	1.80	1.79	1.78	1.77	1.76	1.76
30	1.75	1.74	1.73	1.72	1.71	1.70	1.69	1.69	1.68	1.67
31	1.66	1.65	1.64	1.63	1.62	1.61	1.60	1.60	1.59	1.58
32	1.57	1.56	1.55	1.54	1.53	1.52	1.51	1.50	1.49	1.48
33	1.48	1.47	1.46	1.45	1.44	1.43	1.42	1.41	1.40	1.39
34	1.38	1.37	1.36	1.35	1.34	1.33	1.32	1.31	1.30	1.29
35	1.28	1.27	1.26	1.25	1.24	1.23	1.22	1.21	1.20	1.19
36	1.18	1.17	1.16	1.15	1.14	1.13	1.12	1.11	1.10	1.09
37	1.08	1.07	1.06	1.05	1.04	1.03	1.02	1.00	0.99	0.98
38	0.97	0.96	0.95	0.94	0.93	0.92	0.91	0.90	0.89	0.88
39	0.86	0.85	0.84	0.83	0.82	0.81	0.80	0.79	0.78	0.76
40	0.75									

**AG2.5 Refractometer Calibration Fluid - °Brix Temperature Relationship**

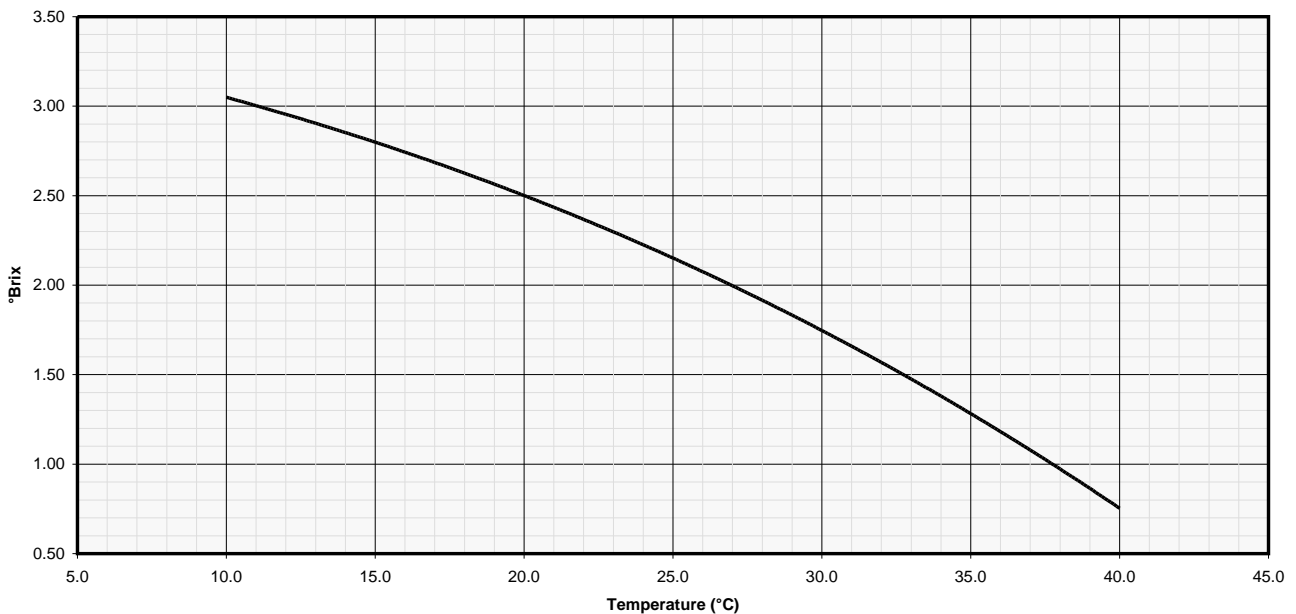

Code: 90-303 Issue: 02 Revision: A



**Bellingham + Stanley Ltd.**

Longfield Road  
Tunbridge Wells  
Kent, TN2 3EY, UK  
Telephone: +44 (0) 1892 500400  
Fax: +44 (0) 1892 543115

**Bellingham + Stanley Inc.**

90 Horizon Drive  
Suwanee  
GA 30024, USA  
Telephone: 678 804 5730  
Fax: 678 804 5729