


AG7.5 Refractometer Calibration Fluid Refractive Index Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	1.34496	1.34495	1.34494	1.34493	1.34492	1.34492	1.34491	1.34490	1.34489	1.34488
11	1.34487	1.34487	1.34486	1.34485	1.34484	1.34483	1.34482	1.34481	1.34481	1.34480
12	1.34479	1.34478	1.34477	1.34476	1.34475	1.34474	1.34474	1.34473	1.34472	1.34471
13	1.34470	1.34469	1.34468	1.34467	1.34466	1.34465	1.34465	1.34464	1.34463	1.34462
14	1.34461	1.34460	1.34459	1.34458	1.34457	1.34456	1.34455	1.34454	1.34453	1.34452
15	1.34451	1.34451	1.34450	1.34449	1.34448	1.34447	1.34446	1.34445	1.34444	1.34443
16	1.34442	1.34441	1.34440	1.34439	1.34438	1.34437	1.34436	1.34435	1.34434	1.34433
17	1.34432	1.34431	1.34430	1.34429	1.34428	1.34427	1.34426	1.34425	1.34424	1.34423
18	1.34422	1.34421	1.34420	1.34419	1.34418	1.34417	1.34416	1.34415	1.34414	1.34413
19	1.34412	1.34410	1.34409	1.34408	1.34407	1.34406	1.34405	1.34404	1.34403	1.34402
20	1.34401	1.34400	1.34399	1.34398	1.34397	1.34395	1.34394	1.34393	1.34392	1.34391
21	1.34390	1.34389	1.34388	1.34387	1.34385	1.34384	1.34383	1.34382	1.34381	1.34380
22	1.34379	1.34378	1.34376	1.34375	1.34374	1.34373	1.34372	1.34371	1.34369	1.34368
23	1.34367	1.34366	1.34365	1.34364	1.34362	1.34361	1.34360	1.34359	1.34358	1.34357
24	1.34355	1.34354	1.34353	1.34352	1.34351	1.34349	1.34348	1.34347	1.34346	1.34344
25	1.34343	1.34342	1.34341	1.34340	1.34338	1.34337	1.34336	1.34335	1.34333	1.34332
26	1.34331	1.34330	1.34328	1.34327	1.34326	1.34325	1.34323	1.34322	1.34321	1.34319
27	1.34318	1.34317	1.34316	1.34314	1.34313	1.34312	1.34310	1.34309	1.34308	1.34306
28	1.34305	1.34304	1.34303	1.34301	1.34300	1.34299	1.34297	1.34296	1.34295	1.34293
29	1.34292	1.34290	1.34289	1.34288	1.34286	1.34285	1.34284	1.34282	1.34281	1.34280
30	1.34278	1.34277	1.34275	1.34274	1.34273	1.34271	1.34270	1.34268	1.34267	1.34266
31	1.34264	1.34263	1.34261	1.34260	1.34259	1.34257	1.34256	1.34254	1.34253	1.34251
32	1.34250	1.34248	1.34247	1.34246	1.34244	1.34243	1.34241	1.34240	1.34238	1.34237
33	1.34235	1.34234	1.34232	1.34231	1.34229	1.34228	1.34226	1.34225	1.34223	1.34222
34	1.34220	1.34219	1.34217	1.34216	1.34214	1.34213	1.34211	1.34210	1.34208	1.34207
35	1.34205	1.34204	1.34202	1.34200	1.34199	1.34197	1.34196	1.34194	1.34193	1.34191
36	1.34189	1.34188	1.34186	1.34185	1.34183	1.34181	1.34180	1.34178	1.34177	1.34175
37	1.34173	1.34172	1.34170	1.34169	1.34167	1.34165	1.34164	1.34162	1.34160	1.34159
38	1.34157	1.34155	1.34154	1.34152	1.34150	1.34149	1.34147	1.34145	1.34144	1.34142
39	1.34140	1.34139	1.34137	1.34135	1.34134	1.34132	1.34130	1.34128	1.34127	1.34125
40	1.34123									

AG7.5 Refractometer Calibration Fluid - R.I. Temperature Relationship

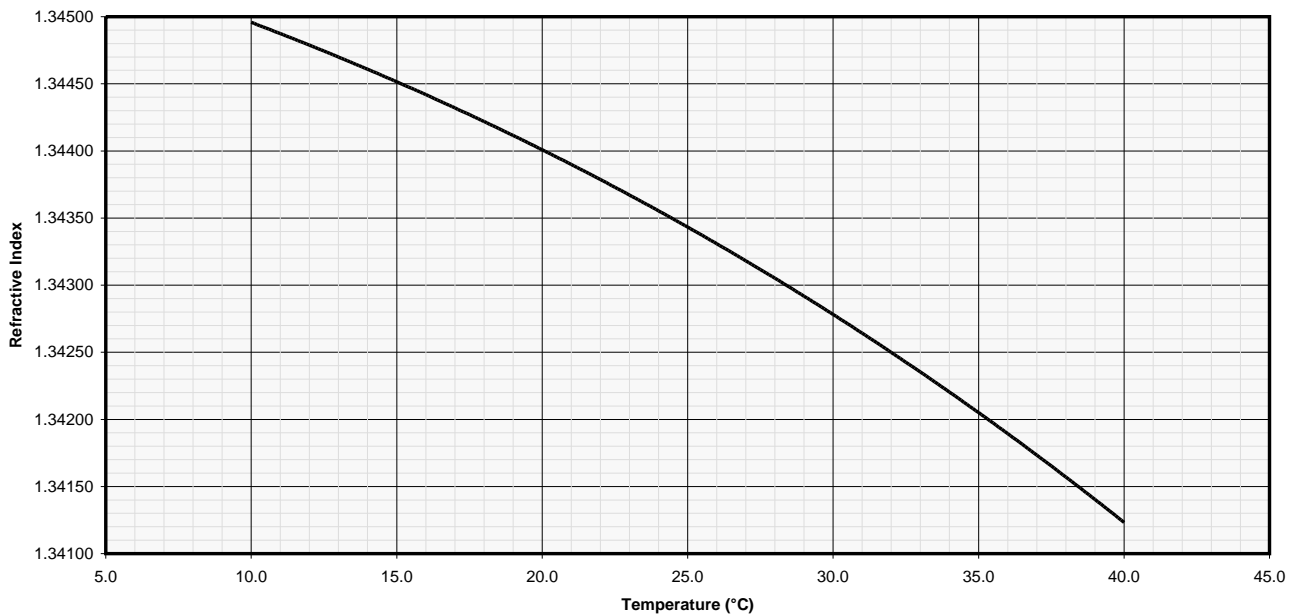

Code: 90-305 Issue: 02 Revision: A



Bellingham + Stanley Ltd.

Longfield Road
Tunbridge Wells
Kent, TN2 3EY, UK
Telephone: +44 (0) 1892 500400
Fax: +44 (0) 1892 543115


Bellingham + Stanley Inc.

90 Horizon Drive
Suwanee
GA 30024, USA
Telephone: 678 804 5730
Fax: 678 804 5729

AG7.5 Refractometer Calibration Fluid °Brix Temperature Relationship

Temperature (°C)	0.0	0.1	0.2	0.3	0.4	0.5	0.6	0.7	0.8	0.9
10	8.12	8.12	8.11	8.11	8.10	8.10	8.09	8.08	8.08	8.07
11	8.07	8.06	8.06	8.05	8.05	8.04	8.03	8.03	8.02	8.02
12	8.01	8.01	8.00	7.99	7.99	7.98	7.98	7.97	7.96	7.96
13	7.95	7.95	7.94	7.94	7.93	7.92	7.92	7.91	7.91	7.90
14	7.89	7.89	7.88	7.87	7.87	7.86	7.86	7.85	7.84	7.84
15	7.83	7.83	7.82	7.81	7.81	7.80	7.79	7.79	7.78	7.77
16	7.77	7.76	7.76	7.75	7.74	7.74	7.73	7.72	7.72	7.71
17	7.70	7.70	7.69	7.68	7.68	7.67	7.66	7.66	7.65	7.64
18	7.64	7.63	7.62	7.62	7.61	7.60	7.60	7.59	7.58	7.57
19	7.57	7.56	7.55	7.55	7.54	7.53	7.53	7.52	7.51	7.50
20	7.50	7.49	7.48	7.48	7.47	7.46	7.45	7.45	7.44	7.43
21	7.42	7.42	7.41	7.40	7.40	7.39	7.38	7.37	7.37	7.36
22	7.35	7.34	7.34	7.33	7.32	7.31	7.30	7.30	7.29	7.28
23	7.27	7.27	7.26	7.25	7.24	7.24	7.23	7.22	7.21	7.20
24	7.20	7.19	7.18	7.17	7.16	7.16	7.15	7.14	7.13	7.12
25	7.12	7.11	7.10	7.09	7.08	7.07	7.07	7.06	7.05	7.04
26	7.03	7.03	7.02	7.01	7.00	6.99	6.98	6.97	6.97	6.96
27	6.95	6.94	6.93	6.92	6.91	6.91	6.90	6.89	6.88	6.87
28	6.86	6.85	6.85	6.84	6.83	6.82	6.81	6.80	6.79	6.78
29	6.77	6.77	6.76	6.75	6.74	6.73	6.72	6.71	6.70	6.69
30	6.68	6.67	6.67	6.66	6.65	6.64	6.63	6.62	6.61	6.60
31	6.59	6.58	6.57	6.56	6.55	6.54	6.53	6.52	6.51	6.50
32	6.50	6.49	6.48	6.47	6.46	6.45	6.44	6.43	6.42	6.41
33	6.40	6.39	6.38	6.37	6.36	6.35	6.34	6.33	6.32	6.31
34	6.30	6.29	6.28	6.27	6.26	6.25	6.24	6.23	6.22	6.21
35	6.20	6.19	6.18	6.16	6.15	6.14	6.13	6.12	6.11	6.10
36	6.09	6.08	6.07	6.06	6.05	6.04	6.03	6.02	6.01	6.00
37	5.98	5.97	5.96	5.95	5.94	5.93	5.92	5.91	5.90	5.89
38	5.88	5.86	5.85	5.84	5.83	5.82	5.81	5.80	5.79	5.77
39	5.76	5.75	5.74	5.73	5.72	5.71	5.70	5.68	5.67	5.66
40	5.65									

AG7.5 Refractometer Calibration Fluid - °Brix Temperature Relationship

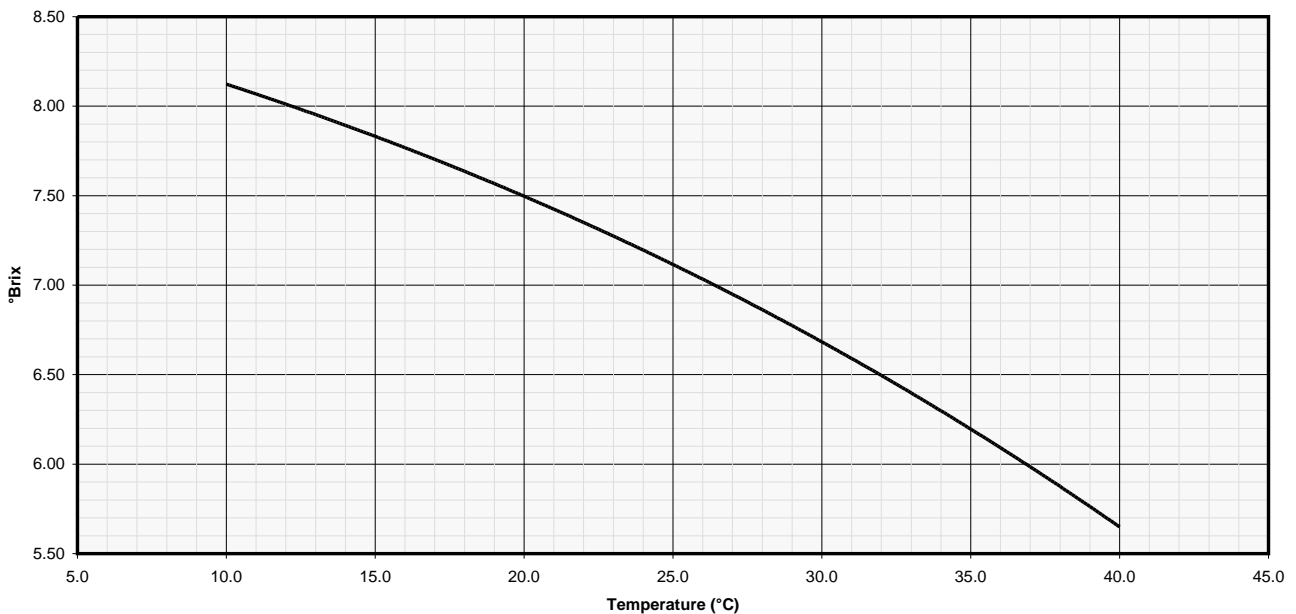

Code: 90-305 Issue: 02 Revision: A



Bellingham + Stanley Ltd.

Longfield Road
Tunbridge Wells
Kent, TN2 3EY, UK
Telephone: +44 (0) 1892 500400
Fax: +44 (0) 1892 543115

Bellingham + Stanley Inc.

90 Horizon Drive
Suwanee
GA 30024, USA
Telephone: 678 804 5730
Fax: 678 804 5729